

Analysis of Selenium in Difficult Samples

Michael Paul
Thermo Fisher Scientific GmbH, Im Steingrund 4-6, Dreieich, Germany

Introduction

Selenium is an essential element for humans and most other living organisms; its most relevant chemical form in biological systems is Selenocysteine, an amino acid found in a variety of enzymes like the Glutathion peroxidases that protect body tissues from oxidative stress. Low Selenium intake in humans may lead in to serious illnesses. High regular doses, however, can be highly toxic.

For drinking water, foodstuff, and many environmental regulations, limit values have been implemented that must not be exceeded. Therefore, the analysis of Selenium has become an important application in routine laboratory work.

ICP-MS is today's method of choice for multi-element analysis. With its unique features, e.g. detection power, sample throughput and dynamic working range, ICP-MS appears to be the perfect analytical tool for all detectable elements. However, attention must be directed to both spectral and non-spectral interferences that can impact on the accuracy of Selenium analysis.

Interferences on Selenium

Non-spectral interferences

Non-spectral interferences on Selenium are related to its high ionization potential (I.P.=9.75 eV). Under the standard operating conditions of an Argon-based ICP, the ionization degree of Selenium is limited to a few percent, leading to poor sensitivity. Additionally, the distribution of total element sensitivity across several isotopes (Figure 1.) makes it challenging to reach detection limits for some analytical requirements. As well as the low Selenium sensitivity in simple aqueous solutions, sample matrix can contribute to either poorer or better ionization. In a previous work¹ the impact of refractory matrix elements and the presence of Carbon was investigated. An increase of Selenium ionization and improved matrix tolerance was found when either CH₄ was added to the nebulizer gas flow or high-purity organic solvents, e.g. 2-Propanol, was continuously mixed with the sample flow. Compared with aqueous solutions the introduction of Carbon to the ICP can improve sensitivity of Selenium by a factor of up to 8.

Spectral interferences

Selenium analysis can suffer from a number of spectral interferences. Even in aqueous solutions without additional sample matrix, significant overlaps of ArAr⁺ occur on all Selenium isotopes. With modern reaction/collision cell designs they can be significantly attenuated. The best working mechanism was found in reaction cell mode based on 8% H₂/He premixed reaction gas (Figure 1 and 2).

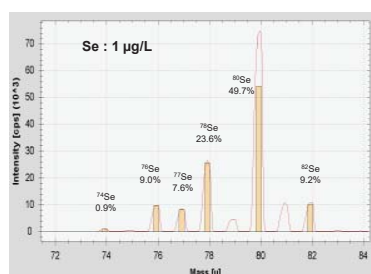


FIGURE 1. Selenium isotopes

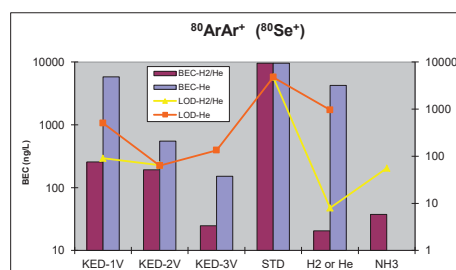


FIGURE 2. Interference removal on ⁸⁰Se

In addition to the predominating ArAr⁺ molecular ions, there are some other interfering species affecting the accurate analysis of Selenium. Table 1 shows a list of typical sample-specific interfering candidates. Krypton may be difficult to control, because this gas is a contaminant of the Argon used for the ICP, namely liquid Argon may show high levels of Krypton. The listed molecular ions can be attenuated successfully by KED while sacrificing Selenium sensitivity.

Doubly charged Rare Earth Elements (REE) cannot be removed or attenuated by collision or reaction cell processes. Although not commonly present, in particular Gadolinium has to be considered in several applications. In clinical samples, namely whole blood and serum, Gadolinium can be present due to the application of Gadoteric acid and related contrast media for MRI examinations. Environmental samples, especially surface and urban waste waters, are increasingly contaminated with Gadolinium due to MRIs conducted in hospitals. Also in other biological materials, e.g. plant leaves, Gadolinium is sometimes present, either by co-absorption from soil or environmental contamination.

Mass (a.m.u.)	Selenium Interference	relative abundance (%)
74	Ge	36.5
74	ArS	4.2
74	FeOH	2.2
74	Sm ⁺⁺	11.3
76	Ge	7.8
76	Sm ⁺⁺	26.7
77	ArCl	24.1
77	Sm ⁺⁺	22.7
78	Gd ⁺⁺	20.5
78	Kr	0.4
80	ArCa	96.6
80	Gd ⁺⁺	21.9
80	Kr	2.3
82	BrH	49.3
82	Kr	11.6
82	ArCa	0.6
82	Dy ⁺⁺	28.2

TABLE 1. Interferences on Se isotopes

Solving the Gd⁺⁺ problem

Instrumentation

All investigations were carried out using a Thermo Scientific™ iCAP™ Qc ICP-MS (Thermo Fisher Scientific, Bremen, Germany) in standard configuration. For sample introduction, a FAST module (Elemental Scientific, Omaha, NE, USA) equipped with a 1 mL sample loop was used. ¹⁰³Rh was used for internal standardization and mixed online with the sample flow combined with 10 per cent (v/v) semiconductor grade 2-Propanol, (Alfa Aesar GmbH & Co. KG, Karlsruhe, Germany). The operating conditions of the iCAP Qc ICP-MS are listed in Table 2.

Reaction cell with Oxygen

Oxygen can help transfer native Selenium into its oxides which in turn can be analyzed at masses 16 a.m.u. higher, e.g. ⁷⁸Se¹⁶O⁺ and ⁸⁰Se¹⁶O⁺, respectively. The SeO⁺ molecular ions are isobaric with Molybdenum isotopes. Although in some cases Molybdenum can be completely oxidized to either MoO⁺ or MoOO⁺, this effect is strongly dependent on the reaction cell settings and on the Molybdenum concentration present in the sample. Not enough Oxygen in the cell and the Molybdenum oxidation will be incomplete. Too high Oxygen flows will reduce Selenium sensitivity and sacrifice detection power.

Reaction cell with Hydrogen and interference correction

The use of Hydrogen is one of the best studied regimes in reaction cell technology. It can eliminate ArAr⁺ signals very efficiently, but is not capable of removing the Gd⁺⁺ overlap on Selenium isotopes. However, at a mass resolution of ca. 0.4 a.m.u. ¹⁵⁵Gd⁺⁺ can be mass resolved from the signals at 77 and 78 a.m.u. (see Figure 3).

Parameter	Units	KED	10% O ₂ / He	8% H ₂ / He	STD
Sampling Depth	mm	5	5	5	5
Plasma Power	W	1550	1550	1550	1550
Cool Flow	L/min	14	14	14	14
Auxiliary Flow	L/min	0,65	0,65	0,65	0,65
Nebulizer Flow	L/min	0,84	0,84	0,84	0,84
CCT Bias	V	-21	-13	-10,01	-2
Pole Bias	V	-18	-20	-16	-1
CCT1 Flow	mL/min	5,0	0,0	5,0	0,0
CCT2 Flow	mL/min	0,0	3,4	0,0	0,0

TABLE 2. Settings for measurement modes.

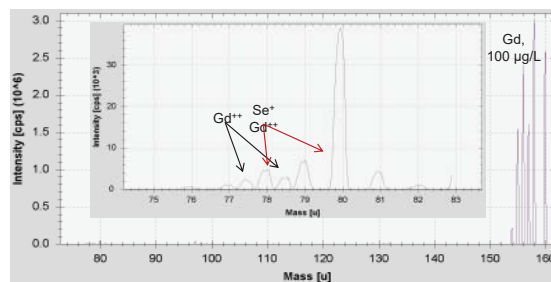


FIGURE 3. Mass resolution of Gd²⁺ interferences from Selenium isotopes

Since the abundances of ¹⁵⁵Gd and ¹⁵⁶Gd are well known and it can be assumed that all Gadolinium isotopes form the same level of doubly charged ions, a mathematical interference correction can be applied to subtract the Gd⁺⁺ contribution from the signal measured at mass 78 and obtain the net Selenium intensity.

Results

Although Selenium analysis can be difficult when Molybdenum and Gadolinium are also present in the sample, there is an easy way to accomplish accurate analysis. Table 3 lists the results from a multi-mode analysis of variant test samples as well as a NIST certified reference material², known for problematic Selenium analysis. Test solutions with different spike amounts of Molybdenum and Gadolinium demonstrate the applicability of the operating conditions of an iCAP Qc ICP-MS and tolerance against high excess of these interfering species. Highlighted in green are well-matching results, while Selenium recoveries in NIST-1547 highlighted in red indicate unacceptable agreement. Reactive mode with H₂/He and the application of interference correction based on half-mass measurement of ¹⁵⁵Gd⁺⁺ results in superb detection limits and excellent agreement with certified values as well as high tolerance against Gadolinium spikes on the analytical results for Selenium.

Measurement Mode	NIST-1547 certified (µg/kg)	STD			8% H ₂ / He				KED				10% O ₂ / He	
		⁷⁷ Se	⁷⁸ Se	⁸² Se	⁷⁷ Se	⁷⁸ Se	⁸⁰ Se	⁸² Se	⁷⁷ Se	⁷⁸ Se	⁸⁰ Se	⁸² Se	⁷⁸ Se ¹⁶ O	⁸⁰ Se ¹⁶ O
10µg/kg Mo		0,002	-0,028	0,000	-0,025	-0,004	-0,104	-0,002	0,033	0,022	0,018	-0,052	68,473	56,259
10µg/kg Gd		0,053	-0,062	0,003	0,063	-0,010	0,045	-0,002	1,127	-0,598	1,650	0,001	0,180	0,164
1µg/kg Se+ 10µg/kg Mo		0,991	0,898	1,015	0,976	0,996	0,953	0,980	0,987	1,041	1,053	1,225	69,925	57,744
1µg/kg Se+ 10µg/kg Gd		1,043	0,858	1,037	1,060	0,991	1,014	0,967	2,245	0,824	2,779	1,120	1,174	1,139
1µg/kg Se+ 100µg/kg Gd		1,664	0,651	1,038	1,814	0,977	2,118	0,968	12,526	-2,342	17,992	1,144	1,035	1,024
1µg/kg Se+10µg/kg Mo&Gd		1,036	0,894	1,042	1,053	0,999	1,010	0,989	2,121	0,938	2,832	1,067	69,023	57,281
NIST 1547 (Peach Leaves)	0.120 +/- 0.009	0,300	0,049	0,172	0,747	0,126	-0,243	0,190	2,972	0,052	0,299	0,857	0,580	0,446
LOD as 3 * SD _{blank}		0,030	0,019	0,014	0,086	0,001	0,061	0,044	0,020	0,024	0,110	0,086	0,047	0,026

TABLE 3. Comparison of analytical results for multi-mode analysis of Selenium.

Conclusions

- The iCAP Q ICP-MS has high detection power for selenium, boosted to up to 8 times the standard sensitivity by the addition of methane gas to the plasma
- High mass resolution capabilities enable the resolution of Gd⁺⁺ interferences from selenium isotopes
- A H₂/He gas mixture provided the best interference reduction and sensitivity combination for selenium analysis, enabling accurate analysis of selenium in samples with high REE content

References

1. M. Paul, Removing spectral interferences in ICP-QMS by collision/reaction cell technology - is there a "best" way ?, Poster presentation at 2011 Winter Conference on Plasma Spectrochemistry, Budapest, Hungary
2. NIST-1547 "Peach Leaves", Certificate of Analysis, National Bureau of Standards & Technology, 1991, Gaithersburg, MD, USA

www.thermofisher.com

©2016 Thermo Fisher Scientific Inc. All rights reserved. ISO is a trademark of the International Standards Organization. FAST is used in trade by Elemental Scientific Inc. All other trademarks are the property of Thermo Fisher Scientific and its subsidiaries. This information is presented as an example of the capabilities of Thermo Fisher Scientific products. It is not intended to encourage use of these products in any manners that might infringe the intellectual property rights of others. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.



Thermo Fisher Scientific,
San Jose, CA USA is
ISO 13485 Certified.

ISO 13485

Africa +43 1 333 50 34 0
Australia +61 3 9757 4300
Austria +43 810 282 206
Belgium +32 53 73 42 41
Canada +1 800 530 8447
China 800 810 5118 (free call domestic)
 400 650 5118

Denmark +45 70 23 62 60
Europe-Other +43 1 333 50 34 0
Finland +358 10 3292 200
France +33 1 60 92 48 00
Germany +49 6103 408 1014
India +91 22 6742 9494
Italy +39 02 950 591

Japan +81 45 453 9100
Korea +82 2 3420 8600
Latin America +1 561 688 8700
Middle East +43 1 333 50 34 0
Netherlands +31 76 579 55 55
New Zealand +64 9 980 6700
Norway +46 8 556 468 00

Russia/CIS +43 1 333 50 34 0
Singapore +65 6289 1190
Spain +34 914 845 965
Sweden +46 8 556 468 00
Switzerland +41 61 716 77 00
UK +44 1442 233555
USA +1 800 532 4752

Thermo
SCIENTIFIC

A Thermo Fisher Scientific Brand